



a xylem brand

CALIBRATION CERTIFICATE

Form No. 830, January 2012

Page 1 of 2

Certificate No: 4330_1083_41102

Product: 4330

Serial No: 1083

Calibration Date:

12.07.2012

Calibration data

Index	Temperature Reference (°C)	[O ₂] Reference (µM)	Phase Reading (°)	Temperature Raw Data (mV)
0	30.363	0.52	60.888	-83.70
1	19.912	0.67	62.197	251.40
2	9.670	1.50	62.974	578.87
3	0.581	3.28	63.570	846.20
4	0.836	24.12	60.110	839.17
5	0.952	46.99	56.818	835.95
6	1.001	68.78	54.091	834.57
7	1.027	108.19	49.937	833.84
8	1.038	152.35	46.182	833.52
9	1.044	229.64	41.171	833.40
10	1.044	330.46	36.531	833.40
11	1.041	431.05	33.211	833.43
12	1.039	552.07	30.259	833.50
13	10.260	17.72	59.017	560.55
14	10.205	33.13	55.923	562.23
15	10.181	51.19	52.803	563.00
16	10.187	85.41	47.971	562.81
17	10.186	117.92	44.359	562.86
18	10.170	176.69	39.433	563.35
19	10.157	268.46	34.210	563.72
20	10.145	341.50	31.339	564.12
21	10.137	440.37	28.478	564.39
22	19.983	11.13	58.386	249.12
23	19.940	25.65	54.384	250.51
24	19.905	41.53	50.765	251.64
25	19.888	67.28	46.079	252.19
26	19.882	94.14	42.293	252.40
27	19.880	146.13	36.971	252.50
28	19.883	212.76	32.438	252.39
29	19.887	285.32	29.102	252.20
30	19.892	356.66	26.767	252.09
31	30.298	7.17	57.834	-81.68
32	30.302	20.94	52.761	-81.80
33	30.301	32.57	49.315	-81.78
34	30.297	53.44	44.419	-81.62
35	30.290	75.07	40.571	-81.40
36	30.285	115.72	35.391	-81.28
37	30.280	172.12	30.753	-81.10
38	30.276	231.58	27.565	-80.99
39	30.271	296.01	25.176	-80.80

Calibration Coefficients

Index	SVUFoilCoef	TempCoef
0	3.38145E-03	2.76984E+01
1	1.40607E-04	-3.15241E-02
2	2.45409E-06	3.39381E-06
3	2.32730E+02	-4.73523E-09
4	-4.67903E-01	0.00000E+00
5	-5.85937E+01	0.00000E+00
6	4.53826E+00	



CALIBRATION CERTIFICATE

Form No. 830, January 2012
Page 2 of 2

Certificate No: 4330_1083_41102


Product: 4330

Serial No: 1083


Calibration Date:

12.07.2012

Oxygen Validation

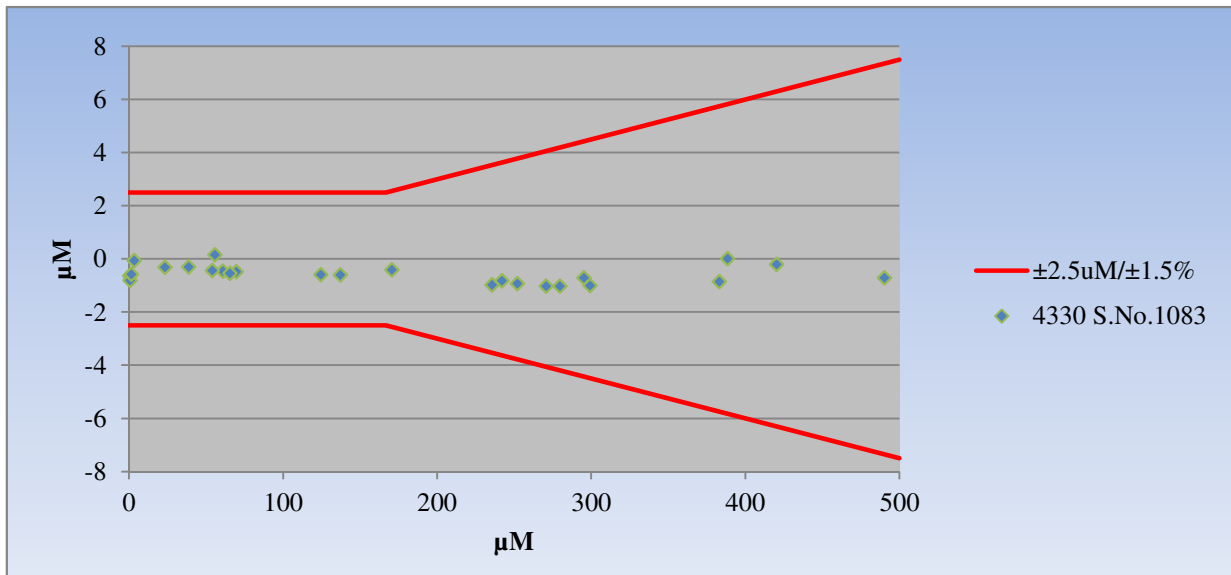

Temperature Validation

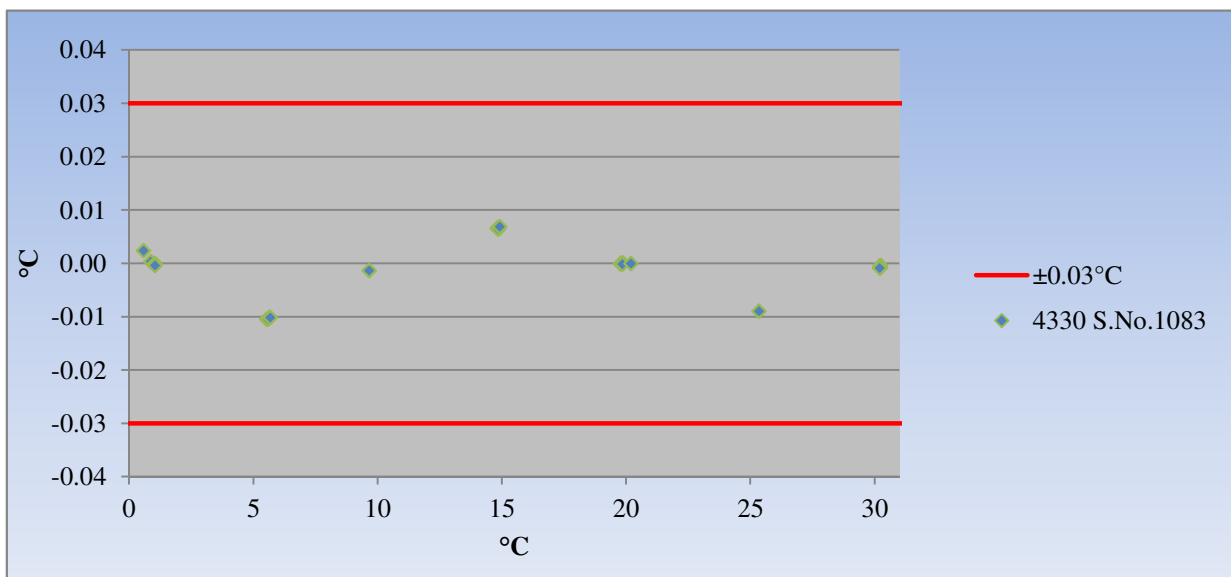

Date: October 30, 2012

Sign:

Jostein Hovdenes
Product Development Manager